



TEST REPORT: MFM-20-24

20W High Reliable Green Medical On Board Type

■ **DESIGN VERIFY TEST**

Output Function Test
Input Function Test
Protection Function Test
Control Function Test
Component Stress Test

■ **SAFETY & E.M.C. TEST**

Safety Test
E.M.C. Test

■ **RELIABILITY TEST**



ENVIRONMENT TEST

DESIGN VERIFY TEST OUTPUT FUNCTION

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	OUTPUT VOLTAGE TOLERANCE (Max)	V1 : 2.0% ~ -2.0%	I/P : 80VAC / 264VAC O/P: FULL / MINLOAD TA: 25°C	V1: 0.79% ~ -0.71%
2	LINE REGULATION (MAX.)	V1 : 0.3% ~ -0.3%	I/P : 80VAC / 264VAC O/P: FULL LOAD TA: 25°C	V1: 0.00% ~ -0.04%
3	LOAD REGULATION(MAX.)	V1 : 0.5% ~ -0.5%	I/P : 230VAC O/P: MIN LOAD ~ FULL LOAD TA: 25°C	V1: 0.04% ~ -0.04%
4	OVER/UNDERSHOOT TEST	< ±5%	I/P : 230VAC O/P: FULL LOAD TA: 25°C	TEST< 4.2 %
	RIPPLE & NOISE(Max)	V1 : 180 mVp-p	I/P : 230VAC O/P: FULL LOAD TA: 25°C	V1 : 57.2 mVp-p

high frequency:


low frequency:

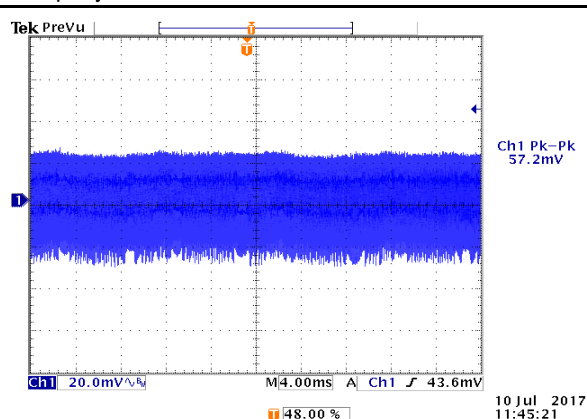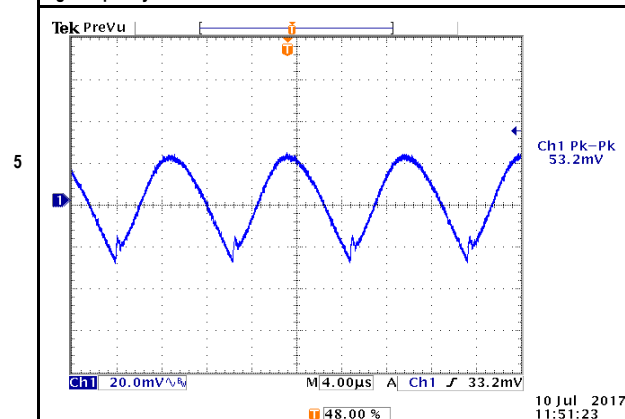

SET UP TIME (MAX.)	230VAC : 1500ms 115VAC : 1500ms	I/P : 230VAC I/P : 115VAC O/P: FULL LOAD TA: 25°C	230VAC : 392ms 115VAC : 168ms
--------------------	------------------------------------	--	----------------------------------


INPUT=230VAC/50HZ @ FULL LOAD

CH1 : Output Voltage CH2 : AC Input Voltage


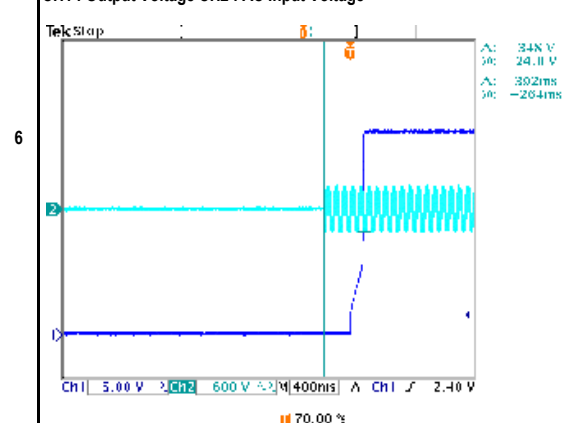




INPUT=115VAC/60HZ @ FULL LOAD

CH1 : Output Voltage CH2 : AC Input Voltage

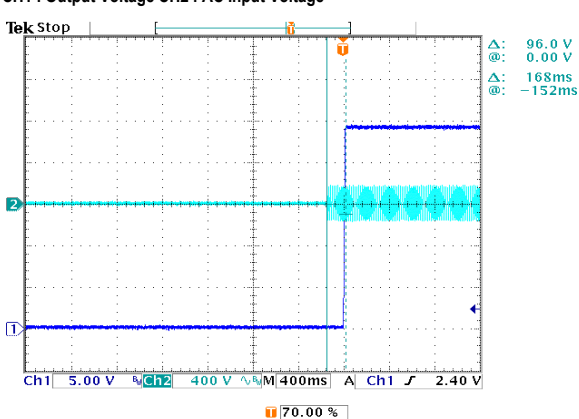

7	RISE TIME (MAX.)	230VAC : 30ms 115VAC : 30ms	I/P : 230VAC I/P : 115VAC O/P: FULL LOAD TA: 25°C	230VAC : 10.0ms 115VAC : 13.2ms
8	HOLD UP TIME (TYP.)	230VAC : 40ms 115VAC : 10ms	I/P : 230VAC I/P : 115VAC O/P: FULL LOAD TA: 25°C	230VAC : 68.0ms 115VAC : 14.0ms
9	DYNAMIC LOAD	V1 : 2400 mVp-p	I/P : 230VAC O/P: (1)Full/Min load 50%duty/120HZ (2)Full/Min load 50%duty/1KHZ TA: 25°C	V1: (1). 980mv (2). 544mv unit:mVp-p

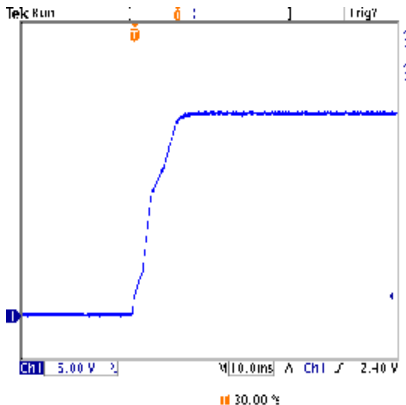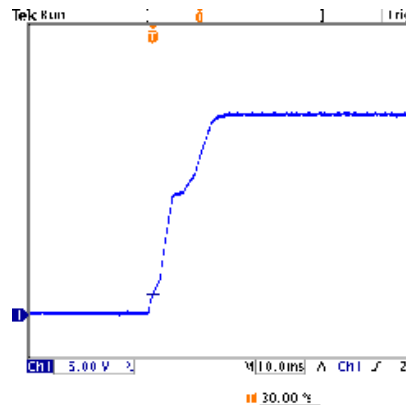
9	INPUT=230VAC/50HZ @ FULL LOAD CH1 : Output Voltage 	INPUT=115VAC/60HZ @ FULL LOAD CH1 : Output Voltage 
---	--	---

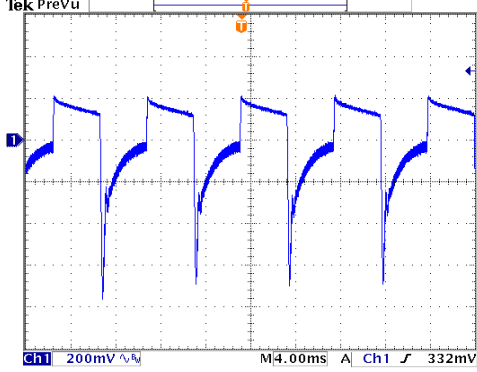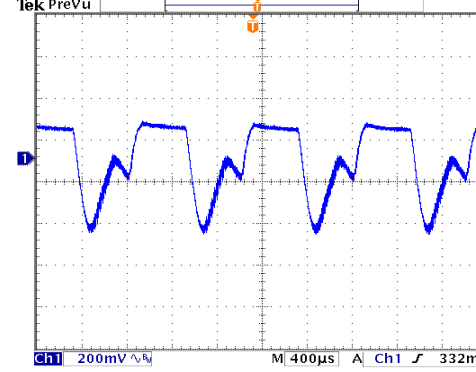9	FULL /MIN LOAD 50%DUTY / 120HZ 	FULL /MIN% LOAD 50%DUTY / 1KHZ 
---	---	--

INPUT FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	INPUT VOLTAGE RANGE	80VAC ~ 264VAC	I/P : TESTING O/P : FULL LOAD Ta : 25°C I/P : LOW-LINE = 97VAC HIGH-LINE = 300VAC O/P : FULL/MIN LOAD ON:30 Sec ; OFF:30 Sec 10MIN (POWER ON/OFF NO DAMAGE)	72.2VAC ~ 264VAC TEST : OK
2	INPUT FREQUENCY RANGE	47HZ ~ 440HZ NO DAMAGE	I/P : 80VAC ~ 264VAC O/P : FULL-MIN LOAD Ta : 25°C	TEST : OK
3	INPUT CURRENT (TYP.)	0.5 / 230VAC 0.75 / 115VAC	I/P : 230VAC I/P : 115VAC O/P : FULL LOAD TA : 25°C	I= 0.188 / 230VAC I= 0.333 / 115VAC
4	LEAKAGE CURRENT	< 80.00μA	I/P : 264VAC O/P : MIN LOAD TA : 25°C	Touch current 46.5 μA
5	NO LOAD POWER CONSUMPTION	< 0.1W	I/P : 230VAC O/P : MIN LOAD TA : 25°C	< 0.059 W
	EFFICIENCY (TYP.)	87.0%	I/P : 230VAC O/P : FULL LOAD TA : 25°C	88.08 %

7

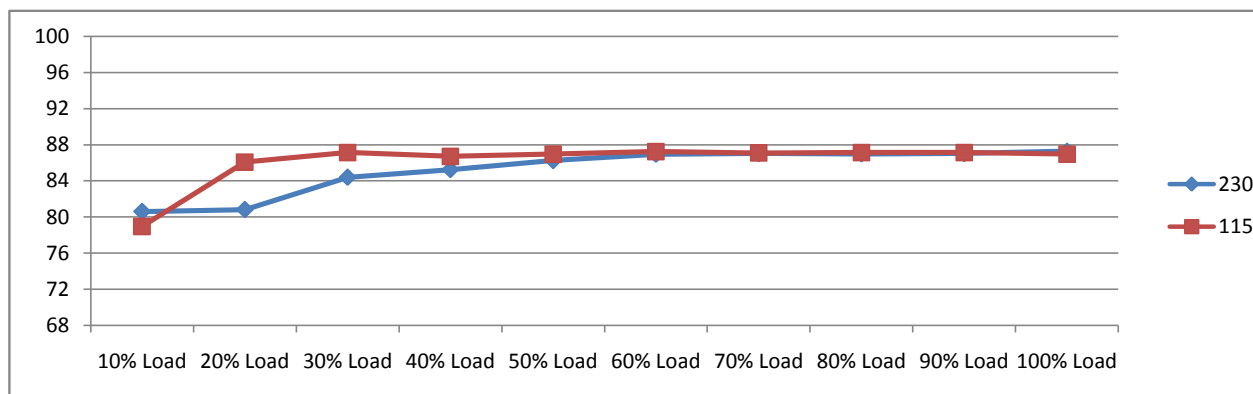

INRUSH CURRENT (TYP.) *

45A / 230VAC
20A / 115VAC
COLD START

I/P : 230VAC
I/P : 115VAC
O/P : FULL LOAD
TA : 25°C

I= 37.0A / 230VAC
I= 17.2A / 115VAC
T50= 264.0us / 230VAC



INPUT=230VAC/50HZ @ FULL LOAD

INPUT=115VAC/50HZ @ FULL LOAD

CH2 : AC Input Voltage CH4 : Input current (1V=1A)

CH2 : AC Input Voltage CH4 : Input current (1V=1A)

8

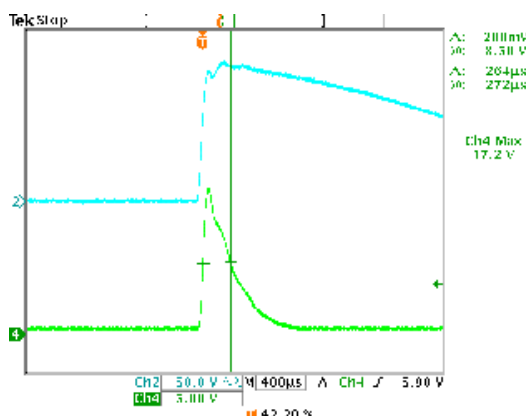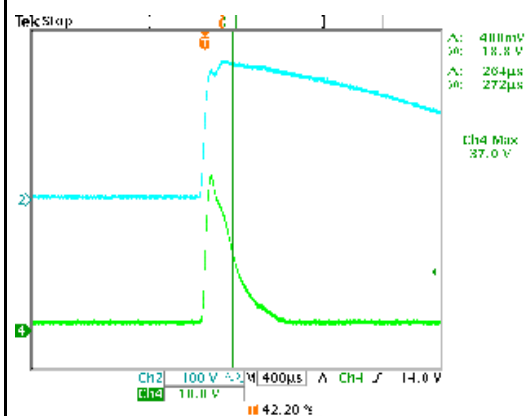



20W High Reliable Green Medical On Board Type MFM-20 series

PROTECTION FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	OVER LOAD PROTECTION	110% ~ 150%	I/P: 264VAC I/P: 230VAC I/P: 100VAC O/P: TESTING Ta: 25°C	141.44% 264VAC 138.11% 230VAC 124.88% 100VAC Hiccup Mode
2	OVER VOLTAGE PROTECTION	27.60V ~ 32.40V	I/P: 80VAC/230VAC/264VAC O/P: MIN LOAD Ta: 25°C	29.10V 264VAC 29.10V 230VAC 29.10V 80VAC Shut off o/p voltage, clamping by zener diode
3	OVER TEMPERATURE PROTECTION	Shut down o/p voltage, recovers automatically after temperature goes down	I/P: 264VAC I/P: 80VAC O/P: FULL LOAD	O.T.P. Active Shut down o/p voltage, recovers automatically after temperature goes down
4	SHORT PROTECTION	SHORT EVERY OUTPUT 1 HOUR NO DAMAGE	I/P: 264VAC I/P: 80VAC O/P: FULL LOAD Ta: 25°C	NO DAMAGE Hiccup Mode

COMPONENT STRESS TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	PWM Power Transistor	U1 Rated : 800V 11.5A	I/P : 267VAC VDS : O/P : (1)Full Load Turn on (2) Output Short (3)Full load continue Ta : 25°C	VIN: 267VAC VDS: (1). 470.00V (2). 436.00V (3). 474.00V
2	O/P MOSFET	Q100 Rated : 200V 5.0A 0 Rated : 0V 0.0A	I/P : 267VAC VDS : O/P : (1)Full Load Turn on (2) Output Short (3)Full load continue Ta : 25°C	Q100 VDS : (1). 118.00V (2). 118.00V (3). 115.00V
3	Input Capacitor	C5 Rated : 33uf 400V	I/P : 267VAC O/P : (1)Full Load Turn on /Off (2)Min load Turn on /Off (3)Full Load /Min load Change (4)Full Load Continue Ta : 25°C	(1). 360.00V (2). 360.00V (3). 358.00V (4). 35.00V
4	Control IC	U1 Rated : 27V (max) -0.3 (min)	I/P : 267VAC O/P : (1)Full Load (2)Output Short (3)O.L.P (4)Low Line No Load Vo(min) Ta : 25°C	U1 (1). 17.60V (2). 16.10V (3). 17.70V (4). 16.00V
9	Clamp Diode	D1 Rated : 1000V 1.0A	I/P : 267VAC O/P : (1)Dynamic Load Full/Min Load (2)Full load continue Ta : 25°C	(1). 434.00V (2). 436.00V

SAFETY & E.M.C. TEST

SAFETY TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	WITHSTAND VOLTAGE	I/P-O/P : 4.000KVAC /min	I/P-O/P: 4.400KVAC /min Ta : 25°C	I/P-O/P: 0.81mA NO DAMAGE
2	ISOLATION RESISTANCE	I/P-O/P : 500VDC>100MΩ	I/P-O/P: 500VDC Ta : 25°C/70%RH	I/P-O/P: 9999.0MΩ NO DAMAGE

E.M.C. TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	HARMONIC	EN61000-3-2 CLASS A	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	PASS



20W High Reliable Green Medical On Board Type MFM-20 series

2	CONDUCTION	EN55011 CLASS B	I/P : 230VAC /50HZ O/P : FULL LOAD / 50% LOAD Ta : 25°C	PASS Test by certified Lab
3	RADIATION	EN55011 CLASS B	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	PASS Test by certified Lab
4	E.S.D	EN61000-4-2 MEDICAL AIR: 15KV / Contact: 8KV	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	CRITERIA A
5	E.F.T	EN61000-4-4 MEDICAL INPUT: 2KV	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	CRITERIA A
6	SURGE	EN61000-4-5 MEDICAL L-N:1KV	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	CRITERIA A

RELIABILITY TEST

READINESS TEST					
NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT	
1	TEMPERATURE RISE TEST	MODEL : MFM-20-24			
		1. ROOM AMBIENT BURN-IN : 1.0hrs			
		IP: 230VAC O/P: 100% LOAD TA= 23.1°C			
		2. HIGH AMBIENT BURN-IN : 1.0hrs			
		IP: 230VAC O/P: 100% LOAD TA= 50.0°C			
		NO.	Positio	ROOM AMBIENT 23.1°C	HIGH AMBIENT Ta: 50.0°C
		1	LF1	56.6°C	80.1°C
		2	C6	69.6°C	91.8°C
		3	C5	65.4°C	100.5°C
		4	U1	99.3°C	115.5°C
		5	T1	78.3°C	106.6°C
		6	C105	48.3°C	89.4°C
		7	Q100	84.9°C	117.5°C
2	OVER LOAD BURN-IN TEST	NO DAMAGE		TEST : OK	
		1 HOUR (MIN)			
		I/P : 230VAC			
		O/P : 130.00% LOAD			
		Ta : 25°C			
3	LOW TEMPERATURE TURN ON TEST	NO DAMAGE		TEST : OK	
		1 HOUR (MIN)			
4	HIGH HUMIDITY HIGH TEMPERATURE HIGH VOLTAGE TEST	I/P : 264VAC / 100VAC		TEST : OK	
		O/P : FULL LOAD			
5	TEMPERATURE COEFFICIENT	Ta : -35.0°C		±0.0091% /(0°C~50°C)	
		HUMIDITY= 95.0% RH			
6	STORAGE TEMPERATURE TEST	I/P : 272VAC		TEST : OK	
		O/P : FULL LOAD			
7	THERMAL SHOCK TEST	Ta : 50°C		TEST : OK	
		HUMIDITY= 95.0% RH			



20W High Reliable Green Medical On Board Type MFM-20 series

8	VIBRATION TEST	1 Carton & 1 Set (1) Waveform : Sine Wave (2) Frequency : 10~500Hz (4) Acceleration : 5G (5) Test Time : 60 min in each axis (X.Y.Z) (6) Ta : 25°C	TEST : OK
9	CAPACITOR LIFE CYCLE	MFM-20-24 :SUPPOSE C105 IS THE MOST CRITICAL COMPONENT (1) I/P : 230VAC O/P : FULL LOAD Ta= 25.0°C LIFE TIME (2) I/P : 230VAC O/P : FULL LOAD Ta= 50.0°C LIFE TIME (3) I/P : 230VAC O/P : 75% LOAD Ta= 50.0°C LIFE TIME (4) I/P : 230VAC O/P : 50% LOAD Ta= 50.0°C LIFE TIME	(1). 357486.3 HRS (2). 33401.7 HRS (3). 57708 HRS (4). 70981 HRS
10	MTBF	Conducted by Parts Stress Analysis Prediction 1210K hrs min. MIL-HDBK-217F (25°C)	
11	DMTBF /Accelerated Life test	Demonstration Mean Time Between Failure (Expected Life): Above 30000HRS @ TA 50°C	

TEST RESULT	TESTER	REVIEW	APPROVAL
PASS	LIUTT		WANGDZ