



TEST REPORT: MPM-30-3.3

30W High Reliable Green Medical Encapsulated Type

■ DESIGN VERIFY TEST

Output Function Test
Input Function Test
Protection Function Test
Control Function Test
Component Stress Test

■ SAFETY & E.M.C. TEST

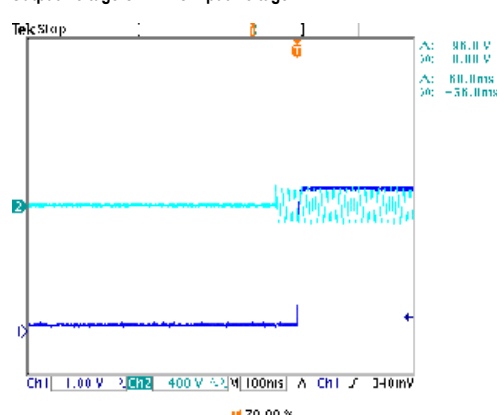
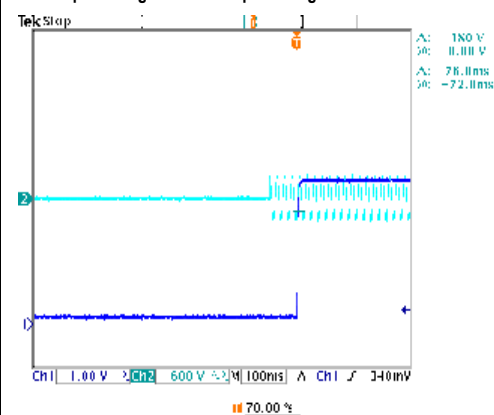
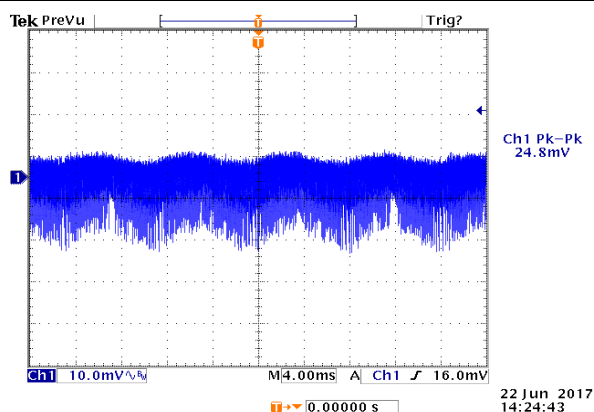
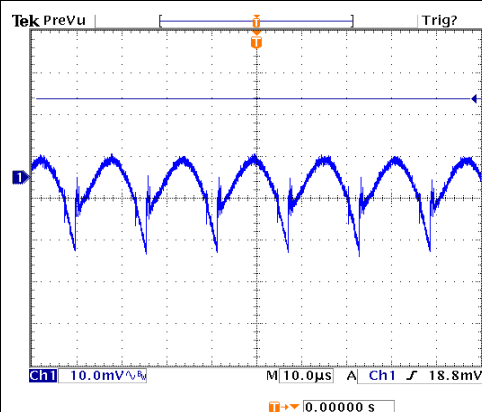
Safety Test
E.M.C. Test

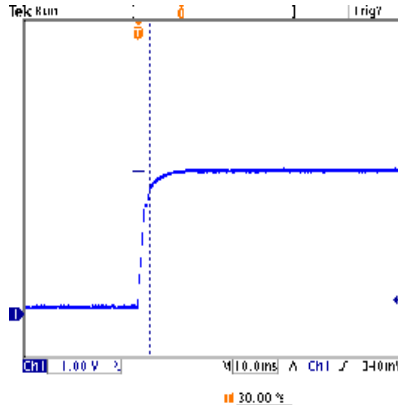
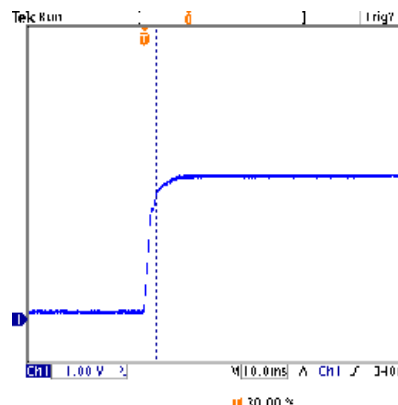
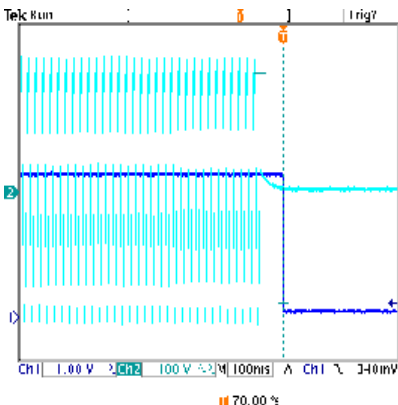
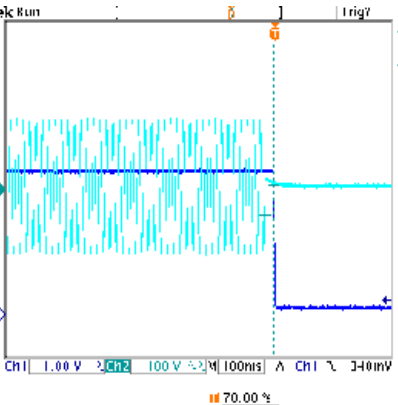
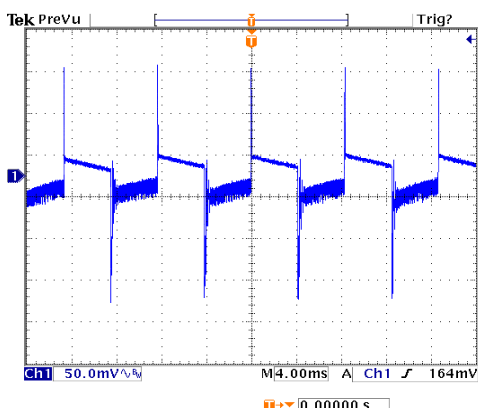
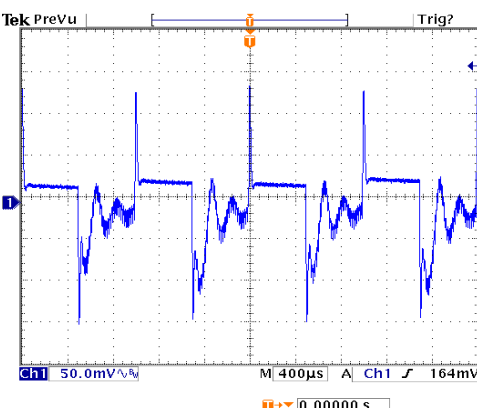
■ RELIABILITY TEST

ENVIRONMENT TEST

DESIGN VERIFY TEST OUTPUT FUNCTION

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	OUTPUT VOLTAGE TOLERANCE (Max)	V1 : 2.0% ~ -2.0%	I/P : 80VAC / 264VAC O/P: FULL / MINLOAD TA: 25°C	V1: 0.00% ~ -0.30%
2	LINE REGULATION (MAX.)	V1 : 0.5% ~ -0.5%	I/P : 80VAC / 264VAC O/P: FULL LOAD TA: 25°C	V1: 0.00% ~ 0.00%
3	LOAD REGULATION(MAX.)	V1 : 1.0% ~ -1.0%	I/P : 230VAC O/P: MIN LOAD ~ FULL LOAD TA: 25°C	V1: 0.00% ~ -0.30%
4	OVER/UNDERSHOOT TEST	< ±15%	I/P : 230VAC O/P: FULL LOAD TA: 25°C	TEST< 3.1 %
5	RIPPLE & NOISE(Max)	V1 : 80 mVp-p	I/P : 230VAC O/P: FULL LOAD TA: 25°C	V1 : 24.8 mVp-p
			high frequency: low frequency:	
6	SET UP TIME (MAX.)	230VAC : 500ms 115VAC : 500ms	I/P : 230VAC I/P : 115VAC O/P: FULL LOAD TA: 25°C	230VAC : 76ms 115VAC : 60ms
		INPUT=230VAC/50HZ @ FULL LOAD CH1 : Output Voltage CH2 : AC Input Voltage	INPUT=115VAC/60HZ @ FULL LOAD CH1 : Output Voltage CH2 : AC Input Voltage	

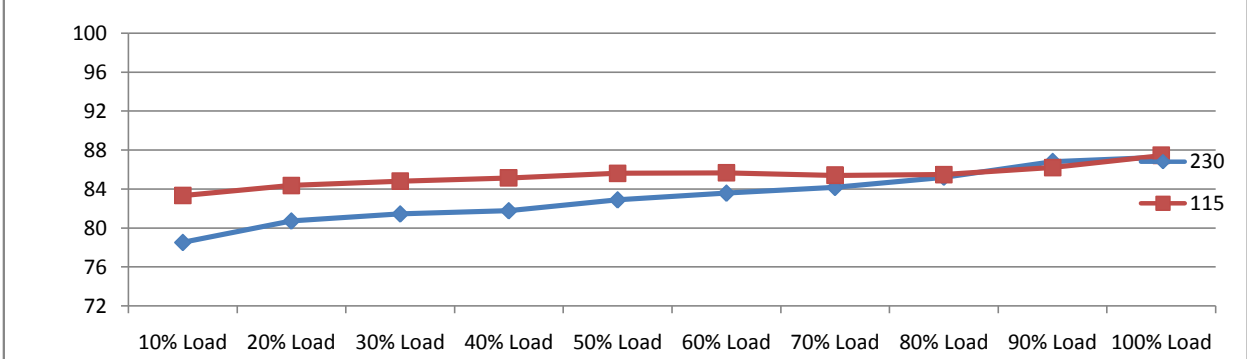
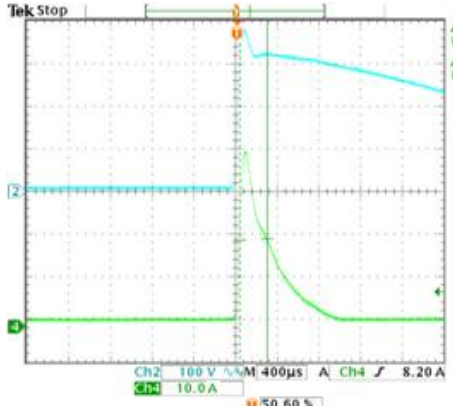
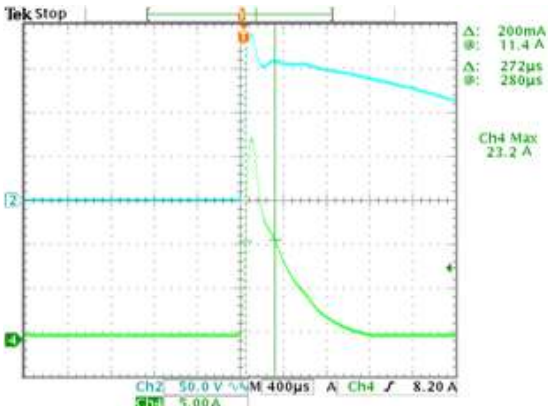


7	RISE TIME (MAX.)	230VAC : 30ms 115VAC : 30ms	I/P : 230VAC I/P : 115VAC O/P: FULL LOAD TA : 25°C	230VAC : 3.0ms 115VAC : 3.0ms
	INPUT=230VAC/50HZ @ FULL LOAD CH1 : Output Voltage		INPUT=115VAC/60HZ @ FULL LOAD CH1 : Output Voltage	
 				
8	HOLD UP TIME (TYP.)	230VAC : 40ms 115VAC : 12ms	I/P : 230VAC I/P : 115VAC O/P: FULL LOAD TA : 25°C	230VAC : 62.0ms 115VAC : 22.0ms
	INPUT=230VAC/50HZ @ FULL LOAD CH1 : Output Voltage CH2 : AC Input Voltage		INPUT=115VAC/60HZ @ FULL LOAD CH1 : Output Voltage CH2 : AC Input Voltage	
 				
9	DYNAMIC LOAD	V1 : 990 mVp-p	I/P : 230VAC O/P: (1)Full/Min load 50%duty/120HZ (2)Full/Min load 50%duty/1KHZ TA : 25°C	V1: (1). 285mv (2). 286mv unit:mVp-p
	FULL /MIN LOAD 50%DUTY / 120HZ		FULL /MIN% LOAD 50%DUTY / 1KHZ	
  22 Jun 2017 14:29:14 22 Jun 2017 14:30:36				

22 Jun 2017
14:29:14

22 Jun 2017
14:30:36

INPUT FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	INPUT VOLTAGE RANGE	80VAC ~ 264VAC	I/P : TESTING O/P : FULL LOAD Ta : 25°C I/P : LOW-LINE = 97VAC HIGH-LINE = 300VAC O/P : FULL/MIN LOAD ON:30 Sec ; OFF:30 Sec 10MIN (POWER ON/OFF NO DAMAGE)	77.0VAC ~ 264VAC TEST : OK
2	INPUT FREQUENCY RANGE	47HZ ~ 63HZ NO DAMAGE	I/P : 80VAC ~ 264VAC O/P : FULL~MIN LOAD Ta : 25°C	TEST : OK
3	INPUT CURRENT (TYP.)	0.50A / 230VAC 0.75A / 115VAC	I/P : 230VAC I/P : 115VAC O/P : FULL LOAD TA : 25°C	I= 0.179A / 230VAC I= 0.303A / 115VAC
4	LEAKAGE CURRENT	< 80.00μA	I/P : 264VAC O/P : MIN LOAD TA : 25°C	Touch current 51.4 μA
5	NO LOAD POWER CONSUMPTION	< 0.075W	I/P : 230VAC O/P : MIN LOAD TA : 25°C	< 0.0571 W
6	EFFICIENCY (TYP.)	82.5%	I/P : 230VAC O/P : FULL LOAD TA : 25°C	87.26 %
				
7	INRUSH CURRENT (TYP.)	45A / 230VAC 25A / 115VAC twidth= 555 us measured at 50% Ipeak COLD START	I/P : 230VAC I/P : 115VAC O/P : FULL LOAD TA : 25°C	I= 41.4A / 230VAC I= 23.2A / 115VAC T50= 264.0us / 230VAC
INPUT=230VAC/50HZ @ FULL LOAD INPUT=115VAC/50HZ @ FULL LOAD CH2 : AC Input Voltage CH4 : Input current CH2 : AC Input Voltage CH4 : Input current				
 				



30W High Reliable Green Medical Encapsulated Type MPM-30 series

PROTECTION FUNCTION TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	OVER LOAD PROTECTION	115% ~ 165%	I/P: 264VAC I/P: 230VAC I/P: 100VAC O/P: TESTING Ta: 25°C	152.20% 264VAC 150.66% 230VAC 142.66% 100VAC Hiccup Mode
2	OVER VOLTAGE PROTECTION	3.50V ~ 4.50V	I/P: 264VAC I/P: 230VAC I/P: 80VAC O/P: MIN LOAD Ta: 25°C	3.80V 264VAC 3.82V 230VAC 3.84V 80VAC Shut down Re- power ON
3	SHORT PROTECTION	SHORT EVERY OUTPUT 1 HOUR NO DAMAGE	I/P: 264VAC I/P: 80VAC O/P: FULL LOAD Ta: 25°C	NO DAMAGE Hiccup Mode ok

COMPONENT STRESS TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	PWM Power Transistor	Q1 Rated : 600V 7.5A	I/P : 267VAC VDS : O/P : (1)Full Load Turn on (2) Output Short (3)Full load continue Ta : 25°C	VIN: 267VAC VDS: (1). 482.00V (2). 484.00V (3). 486.00V
2	O/P MOSFET	Q100 Rated : 100V 80.0A Rated :	I/P : 267VAC VDS : O/P : (1)Full Load Turn on (2) Output Short (3)Full load continue Ta : 25°C	Q100 VDS : (1). 31.40V (2). 28.80V (3). 29.00V
3	Input Capacitor	C5 Rated : 56uf 400V	I/P : 267VAC O/P : (1)Full Load Turn on /Off (2)Min load Turn on /Off (3)Full Load /Min load Change (4)Full Load Continue Ta : 25°C	(1). 372.00V (2). 376.00V (3). 376.00V (4). 372.00V
4	Control IC	U1 Rated : 28V (max) -0.3 (min) 38 -0.3	I/P : 267VAC O/P : (1)Full Load (2)Output Short (3)O.L.P (4)O.V.P (5)Low Line No Load Vo(min) Ta : 25°C	U1 U100 (1). 23.60V 19.2V (2). 12.00V 15.6V (3). 24.00V 19.2 (4). 19.40V 19.6 (5). 17.90V 7.1V
5	Clamp Diode	D5 Rated : 1000V 1.0A	I/P : 267VAC O/P : (1)Dynamic Load Full/Min Load (2)Full load continue Ta : 25°C	(1). 462.00V (2). 458.00V

SAFETY & E.M.C. TEST

SAFETY TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	WITHSTAND VOLTAGE	I/P-O/P : 4.000KVAC /min	I/P-O/P: 4.250KVAC /min Ta : 25°C	I/P-O/P: 1.17mA NO DAMAGE
2	ISOLATION RESISTANCE	I/P-O/P : 500VDC>100MΩ	I/P-O/P: 500VDC Ta : 25°C/70%RH	I/P-O/P: 9999.0MΩ NO DAMAGE

E.M.C. TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT
1	HARMONIC	EN61000-3-2 CLASS A	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	PASS



30W High Reliable Green Medical Encapsulated Type MPM-30 series

2	CONDUCTION	EN55011 CLASS B	I/P : 230VAC /50HZ O/P : FULL LOAD / 50% LOAD Ta : 25°C	PASS Test by certified Lab
3	RADIATION	EN55011 CLASS B	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	PASS Test by certified Lab
4	E.S.D	EN61000-4-2 AIR: 15KV / Contact: 8KV	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	CRITERIA A
5	E.F.T	EN61000-4-4 MEDICAL INPUT: 2KV	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	CRITERIA A
6	SURGE	EN61000-4-5 MEDICAL LINE-LINE:1KV	I/P : 230VAC /50HZ O/P : FULL LOAD Ta : 25°C	CRITERIA A

RELIABILITY TEST

NO	TEST ITEM	SPECIFICATION	TEST CONDITION	RESULT																																																								
1	TEMPERATURE RISE TEST	MODEL : MPM-30-5 1. ROOM AMBIENT BURN-IN : 1.0hrs IP: 230VAC O/P: 100% LOAD TA= 29.2℃ 2. HIGH AMBIENT BURN-IN : 1.0hrs IP: 230VAC O/P: 100% LOAD TA= 61.3℃	<table><tr><th>NO.</th><th>Position</th><th>ROOM AMBIENT 29.2℃</th><th>HIGH AMBIENT Ta: 61.3℃</th></tr><tr><td>1</td><td>LF1</td><td>52.4℃</td><td>81.9℃</td></tr><tr><td>2</td><td>LF2</td><td>53.1℃</td><td>81.9℃</td></tr><tr><td>3</td><td>C5</td><td>57.2℃</td><td>87.5℃</td></tr><tr><td>4</td><td>C40</td><td>61.0℃</td><td>91.5℃</td></tr><tr><td>5</td><td>BD1</td><td>63.1℃</td><td>92.6℃</td></tr><tr><td>6</td><td>R40</td><td>69.8℃</td><td>99.2℃</td></tr><tr><td>7</td><td>T1</td><td>66.4℃</td><td>97.9℃</td></tr><tr><td>8</td><td>Q100</td><td>61.7℃</td><td>93.1℃</td></tr><tr><td>9</td><td>C105</td><td>65.0℃</td><td>96.5℃</td></tr><tr><td>10</td><td>L100</td><td>58.2℃</td><td>89.1℃</td></tr><tr><td>11</td><td>Q1</td><td>63.4℃</td><td>93.8℃</td></tr><tr><td>12</td><td>U1</td><td>61.1℃</td><td>90.7℃</td></tr><tr><td>60</td><td>TA</td><td>29.2℃</td><td>61.3℃</td></tr></table>	NO.	Position	ROOM AMBIENT 29.2℃	HIGH AMBIENT Ta: 61.3℃	1	LF1	52.4℃	81.9℃	2	LF2	53.1℃	81.9℃	3	C5	57.2℃	87.5℃	4	C40	61.0℃	91.5℃	5	BD1	63.1℃	92.6℃	6	R40	69.8℃	99.2℃	7	T1	66.4℃	97.9℃	8	Q100	61.7℃	93.1℃	9	C105	65.0℃	96.5℃	10	L100	58.2℃	89.1℃	11	Q1	63.4℃	93.8℃	12	U1	61.1℃	90.7℃	60	TA	29.2℃	61.3℃	
NO.	Position	ROOM AMBIENT 29.2℃	HIGH AMBIENT Ta: 61.3℃																																																									
1	LF1	52.4℃	81.9℃																																																									
2	LF2	53.1℃	81.9℃																																																									
3	C5	57.2℃	87.5℃																																																									
4	C40	61.0℃	91.5℃																																																									
5	BD1	63.1℃	92.6℃																																																									
6	R40	69.8℃	99.2℃																																																									
7	T1	66.4℃	97.9℃																																																									
8	Q100	61.7℃	93.1℃																																																									
9	C105	65.0℃	96.5℃																																																									
10	L100	58.2℃	89.1℃																																																									
11	Q1	63.4℃	93.8℃																																																									
12	U1	61.1℃	90.7℃																																																									
60	TA	29.2℃	61.3℃																																																									
2	OVER LOAD BURN-IN TEST	NO DAMAGE 1 HOUR (MIN)	I/P : 230VAC O/P : 159.0% LOAD Ta : 25℃	TEST : OK																																																								
3	LOW TEMPERATURE TURN ON TEST	NO DAMAGE 1 HOUR (MIN)	I/P : 264VAC / 100VAC O/P : FULL LOAD Ta : -40.0℃	TEST : OK																																																								
4	HIGH HUMIDITY HIGH TEMPERATURE HIGH VOLTAGE TEST	AFTER 12 HOURS IN CHAMBER ON CONTROL 60℃ NO DAMAGE	I/P : 272VAC O/P : FULL LOAD Ta : 60℃ HUMIDITY= 95.0% RH	TEST : OK																																																								
5	TEMPERATURE COEFFICIENT	±0.03% /℃(0~60℃)	I/P : 230VAC O/P : FULL LOAD	±0.0062% /℃(0~60℃)																																																								
6	STORAGE TEMPERATURE TEST	1. Thermal shock Temperature : -50℃ ~ +125℃ 2. Temperature change rate : 25℃ / MIN 3. Dwell time low and high temperature : 30 MIN/EACH 4. Total test cycle : 100 CYCLE 5. Input/Output condition : STATIC		TEST : OK																																																								
7	THERMAL SHOCK TEST	1. Thermal shock Temperature : -45℃ ~ 65℃ 2. Temperature change rate : 25℃ / MIN 3. Dwell time low and high temperature : 30 MIN/EACH 4. Total test cycle : 16 CYCLE 5. Input/Output condition : 230VAC Full Load AC ON/OFF test turn on 3sec ; turn off 1sec @ 15CYCLE 230VAC Full Load AC ON turn on continue @ 1CYCLE		TEST : OK																																																								



30W High Reliable Green Medical Encapsulated Type MPM-30 series

8	VIBRATION TEST	1 Carton & 1 Set (1) Waveform : Sine Wave (2) Frequency : 10~500Hz (4) Acceleration : 2G (Blank) /5G (ST) (5) Test Time : 60min in each axis (X.Y.Z) (6) Ta : 25°C	TEST : OK
9	CAPACITOR LIFE CYCLE	:SUPPOSE C105 IS THE MOST CRITICAL COMPONENT (1) I/P : 230VAC O/P : FULL LOAD Ta= 25°C LIFE TIME (2) I/P : 230VAC O/P : FULL LOAD Ta= 60°C LIFE TIME (3) I/P : 230VAC O/P : 75% LOAD Ta= 60°C LIFE TIME (4) I/P : 230VAC O/P : 50% LOAD Ta= 60°C LIFE TIME	(1). 215470.2 HRS (2). 30493.9 HRS (3). 34062.7 HRS (4). 54721 HRS
10	MTBF	Conducted by Parts Stress Analysis Prediction 779K hrs min. MIL-HDBK-217F (25°C)	
11	DMTBF /Accelerated Life test	Demonstration Mean Time Between Failure (Expected Life): 30000HRS @ TA 60°C	

TEST RESULT	TESTER	REVIEW	APPROVAL
PASS	LIUTT		WANGDZ